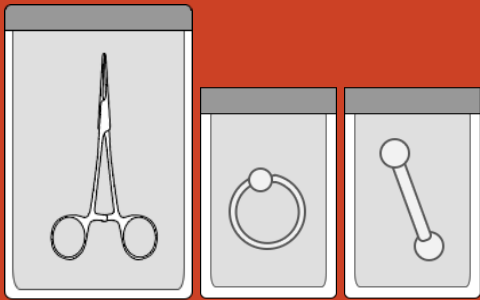
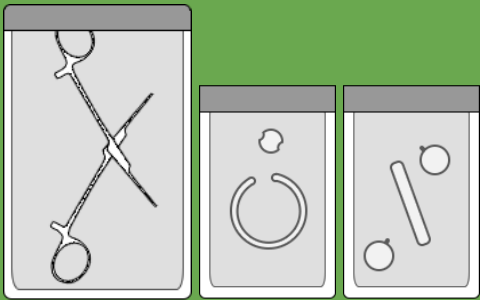
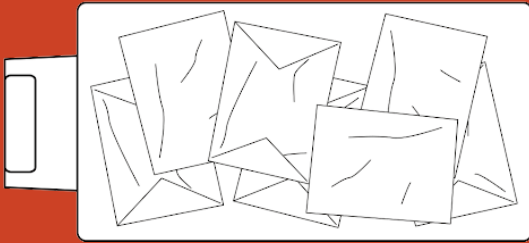
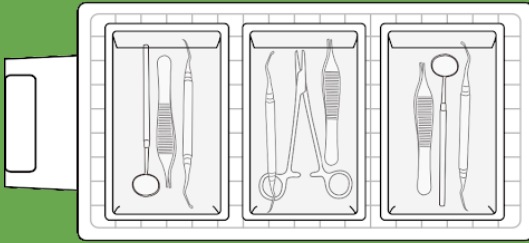
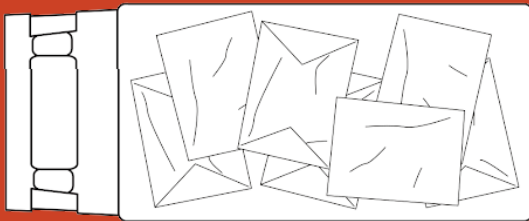
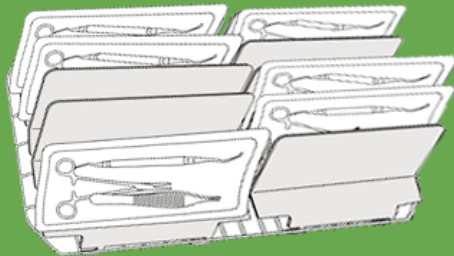
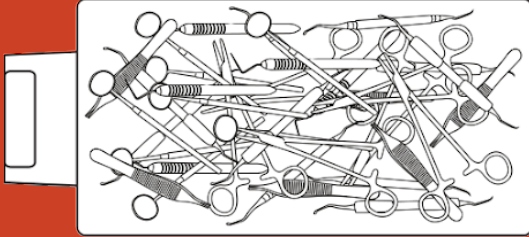
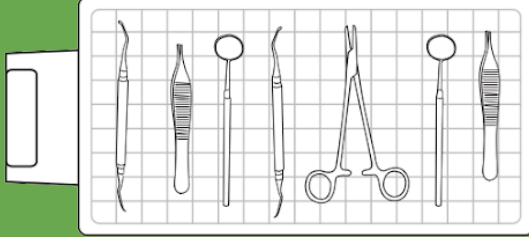


# How to load a steriliser correctly

METHOD	DON'T	DO
Autoclave Pouches		
Statim 2000 Wrapped Cycle		
Statim 5000 Wrapped Cycle		
Statim 2000/5000 Unwrapped Cycle		
Chamber Autoclave Wrapped Cycle	